

Certificate of Performance

TON 2 Reagent



Product Code 984651

984652

Lot Number 0011

Date 07.01.2010


Expiry Date 04.01.2011

Reagent	Lot Number
TON 1	9085
TON 2	0011
TON 3	0012
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.001
2.50	TON 100 11 09	0.183
5.00	TON 100 11 09	0.368
7.69	TON 100 11 09	0.539
10.00	TON 100 11 09	0.695

*serial dilution

Calibration Curve

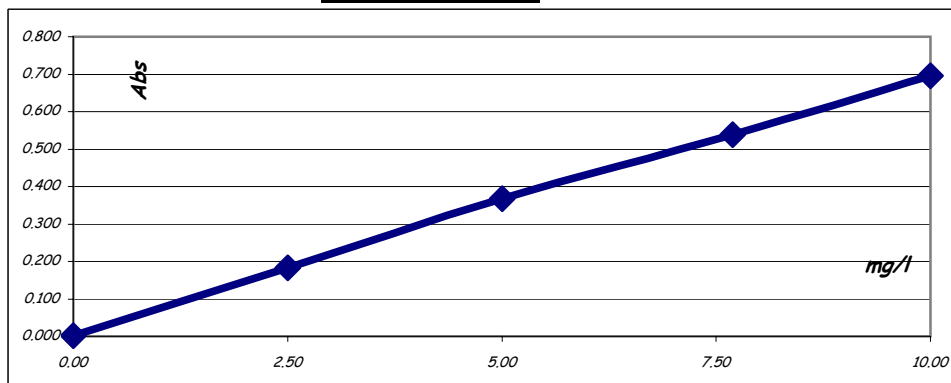

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0728	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0740	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0636	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0675	0.0500 to 0.0700	Pass

Notes
 Store between 2 & 8 °C
 *Stable on Board TON 1 - 1 day
 * TON 2 & TON 3 - 5 days
 Keep Tightly Sealed when not in use.
 Do not return unused portions to container
 Barcode ID- TON 1 758; TON 2 759; TON 3 756
 * Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell