


Certificate of Performance

Phos 2 Reagent



Product Code 984645  
984647  
Lot Number 8083

Date 02.05.2008


Expiry Date 30.04.2009

Reagent	Lot Number
Phos 1	8082
Phos 2	<b>8083</b>
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 02 08	0.152
1	P20 02 08	0.286
1.5	P20 02 08	0.445
2	P20 02 08	0.577

\*serial dilution

Calibration Curve

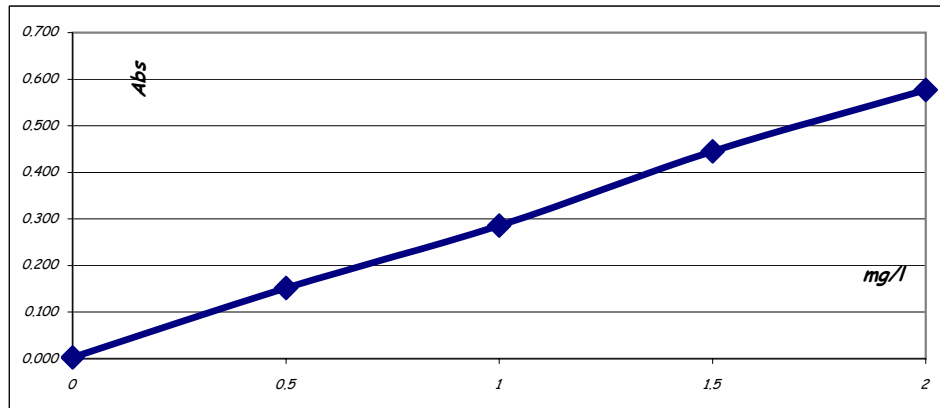

	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	<b>Pass</b>
Sensitivity	Abs/ppm 0.288	0.260 to 0.320	<b>Pass</b>
Regression	0.999	0.990 to 1.001	<b>Pass</b>

Notes Store between 2 & 8 °C  
\*Stable on Board 5 days  
Barcode ID = 765  
\* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell