

Certificate of Performance

Amm 1 Reagent



Product Code 984640 20 ml vial
Lot Number 8086

Date 13.05.2008


Expiry Date 30.04.2009

Reagent	Lot Number
AMM 1	8086
Amm 2	8087
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.020
0.25	AMM 10 03 08	0.220
0.50	AMM 10 03 08	0.420
0.77	AMM 10 03 08	0.642
1.00	AMM 10 03 08	0.824

*serial dilution

Calibration Curve

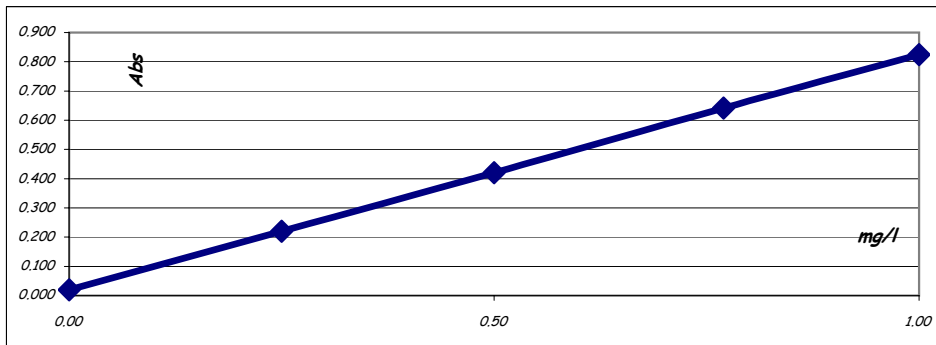

Test	Result	Specification	Pass / Fail
Intercept	0.0192	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8056	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes
 Store between 2 & 8 ° c
 *Stable on Board 1 day
 Barcode ID = 751
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell