

Certificate of Performance

TON 2 Reagent



Product Code 984651 20 ml vial

984652 60 ml vial

Lot Number 8136

Date 22.07.2008


Expiry Date 15.07.2009

Reagent	Lot Number
TON 1	8062
TON 2	8136
TON 3	8142
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.002
2.50	TON 100 05 08	0.185
5.00	TON 100 05 08	0.361
7.69	TON 100 05 08	0.522
10.00	TON 100 05 08	0.658

*serial dilution

Calibration Curve

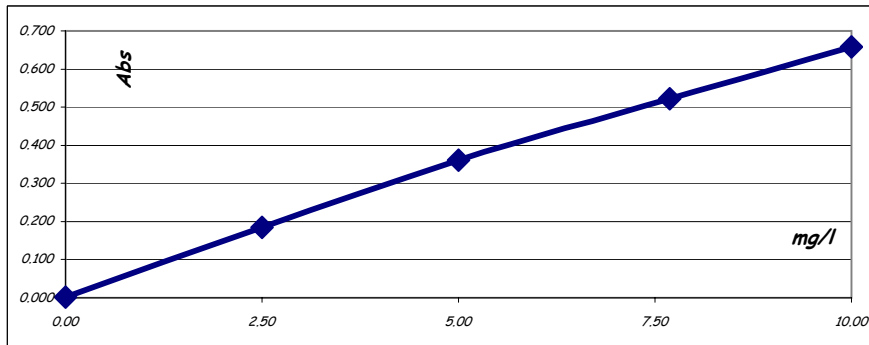

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
0 - 2.50 mg/l	0.0732	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0704	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0599	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0589	0.0500 to 0.0700	Pass

Notes
Store between 2 & 8 °C
*Stable on Board TON 1 - 1 day
* TON 2 & TON 3 - 5 days
Keep Tightly Sealed when not in use.
Do not return unused portions to container
Barcode ID- TON 1 758; TON 2 759; TON 3 756
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell