

Certificate of Performance

Phos 1 Reagent



Product Code 984644 20 ml vial  
984646 60 ml vial  
Lot Number 8137

Date 17.07.2008


Expiry Date 15.07.2009

Reagent	Lot Number
Phos 1	8137
Phos 2	8138
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 02 08	0.151
1	P20 02 08	0.292
1.5	P20 02 08	0.459
2	P20 02 08	0.593

\*serial dilution

**Calibration Curve**

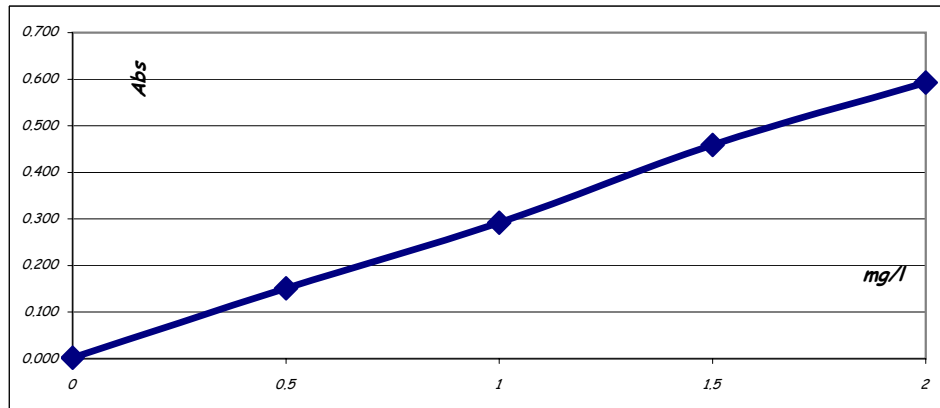

	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.298	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C  
\*Stable on Board 5 days  
Barcode ID = 763  
\* Based on results obtained in our Research Facility

Dr. T. Russell