


Certificate of Performance

Phos 2 Reagent



Product Code 984645 20 ml vial
 984647 60 ml vial
 Lot Number 8138

Date 17.07.2008


Expiry Date 15.07.2009

Reagent	Lot Number
Phos 1	8137
Phos 2	8138
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 02 08	0.151
1	P20 02 08	0.292
1.5	P20 02 08	0.459
2	P20 02 08	0.593

*serial dilution

Calibration Curve

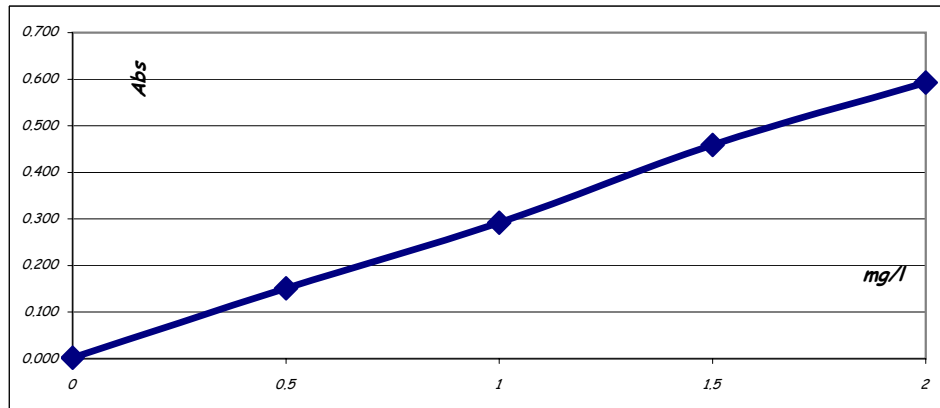

	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.298	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 765
 * Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell