

Certificate of Performance



Chloride Reagent

Product Code 984642 20 ml vial
 984643 60 ml vial
Lot Number 8139


Date 17.07.2008

Expiry Date 15.07.2009

Reagent	Lot Number
Chloride	8139
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.006
250 ppm	CL 4000 05 08	0.322
500 ppm	CL 4000 05 08	0.512
800 ppm	CL 4000 05 08	0.671
1000 ppm	CL 4000 05 08	0.749

Calibration Curve

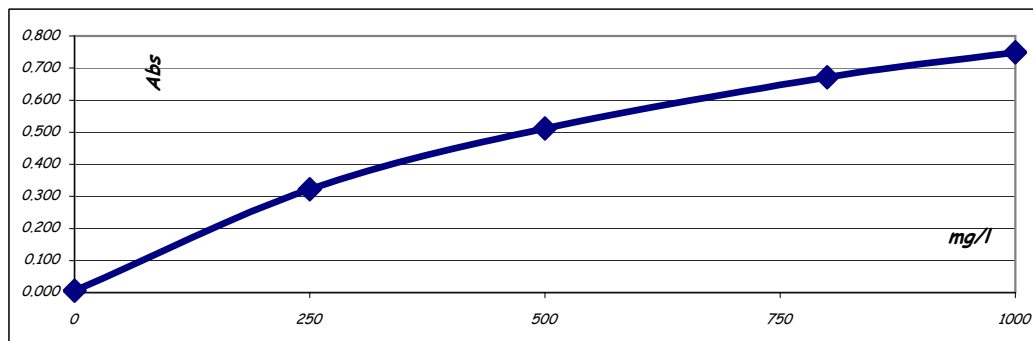

Test	Result	Specification	Pass / Fail
Intercept	0.006	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
	0 - 250 mg/l	0.0013 to 0.0016	Pass
	250 - 500 mg/l	0.0008 to 0.0012	Pass
	500 - 800 mg/l	0.0005 to 0.0010	Pass
	800 - 1000 mg/l	0.0004 to 0.0008	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 5 days
 Barcode ID = 754
 *Based on results obtained in our Research Facility

Dr. T. Russell