

Certificate of Performance

TON 3 Reagent



Product Code 984653 20 ml vial
984654 60 ml vial
Lot Number 8142

Date 22.07.2008


Expiry Date 15.07.2009

Reagent	Lot Number
TON3	8142
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.50	NO2-20 05 08	0.446
1.00	NO2-20 05 08	0.873
1.54	NO2-20 05 08	1.336
2.00	NO2-20 05 08	1.723

*serial dilution

Calibration Curve

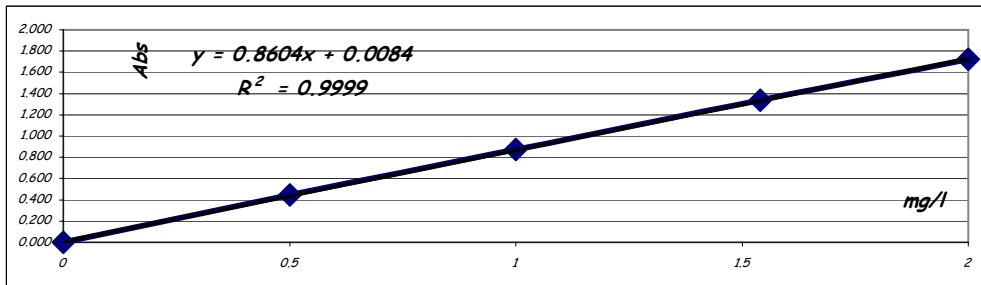

Test	Result	Specification	Pass / Fail
Intercept	0.008	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.860	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 ° c
*Stable on Board 5 days
Barcode ID = 756
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell