

Certificate of Performance

Amm 2 Reagent



Product Code 984641 20 ml vial  
Lot Number 8145

Date 23.07.2008


Expiry Date 15.07.2009

Reagent	Lot Number
AMM 1	8144
Amm 2	8145
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.024
0.25	AMM 10 05 08	0.224
0.50	AMM 10 05 08	0.425
0.77	AMM 10 05 08	0.645
1.00	AMM 10 05 08	0.834

\*serial dilution

Calibration Curve

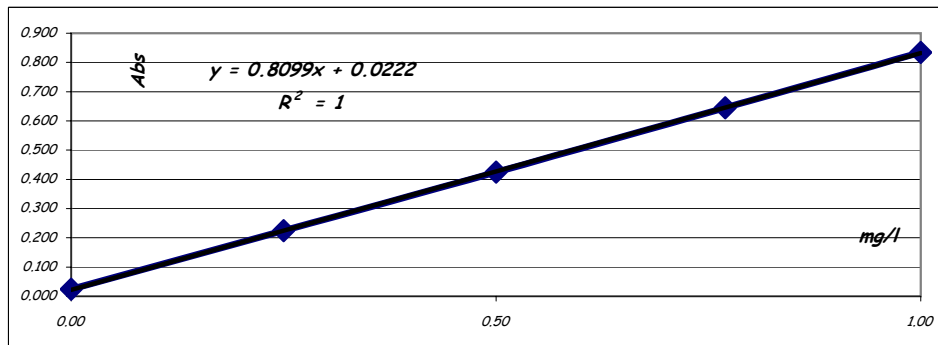

Test	Result	Specification	Pass / Fail
Intercept	0.0222	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8099	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes Store between 2 & 8 ° c  
\*Stable on Board 5 days  
Barcode ID = 752  
\* Based on results obtained in our Research Facility

*Tom Russell.*  
Dr. T. Russell