

Certificate of Performance

TON 3 Reagent



Product Code 984653

984654

Lot Number 8163

Date 01.09.2008


Expiry Date 29.08.2009

Reagent	Lot Number
TON3	8163
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.50	NO2-20 05 08	0.433
1.00	NO2-20 05 08	0.845
1.54	NO2-20 05 08	1.298
2.00	NO2-20 05 08	1.686

\*serial dilution

Calibration Curve

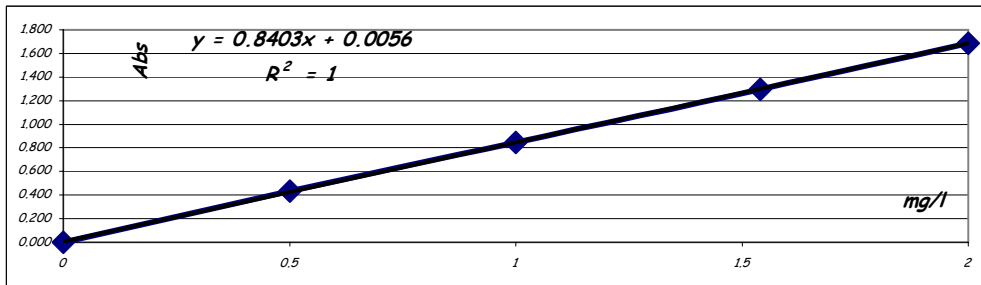

Test	Result	Specification	Pass / Fail
Intercept	0.006	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.840	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 ° c  
\*Stable on Board 5 days  
Barcode ID = 756  
\* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell