

Certificate of Performance

**Amm 1 Reagent**



Product Code 984640  
Lot Number 8167

Date 04.09.2008


Expiry Date 29.08.2009

Reagent	Lot Number
AMM 1	8167
Amm 2	8168
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.018
0.25	AMM 10 05 08	0.217
0.50	AMM 10 05 08	0.428
0.77	AMM 10 05 08	0.641
1.00	AMM 10 05 08	0.835

\*serial dilution

Calibration Curve

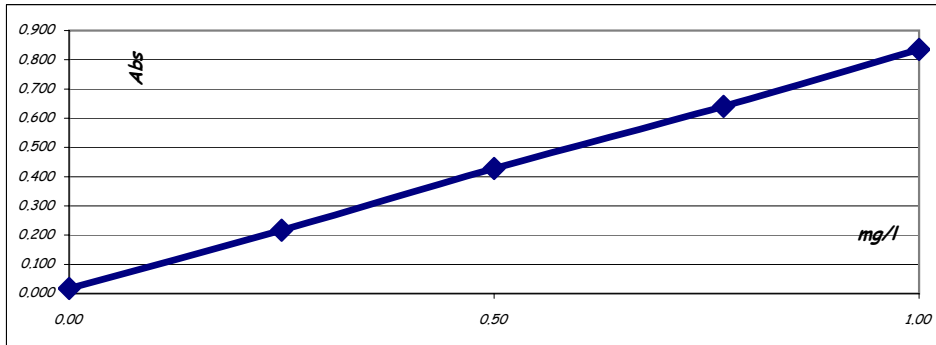

Test	Result	Specification	Pass / Fail
Intercept	0.0163	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8165	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes  
 Store between 2 & 8 ° c  
 \*Stable on Board 1 day  
 Barcode ID = 751  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 Dr. T. Russell