

Certificate of Performance

Amm 2 Reagent



Product Code 984641

Lot Number 8168

Date 04.09.2008


Expiry Date 29.08.2009

Reagent	Lot Number
AMM 1	8167
Amm 2	8168
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.018
0.25	Amm 10 05 08	0.217
0.50	Amm 10 05 08	0.428
0.77	Amm 10 05 08	0.641
1.00	Amm 10 05 08	0.835

*serial dilution

Calibration Curve

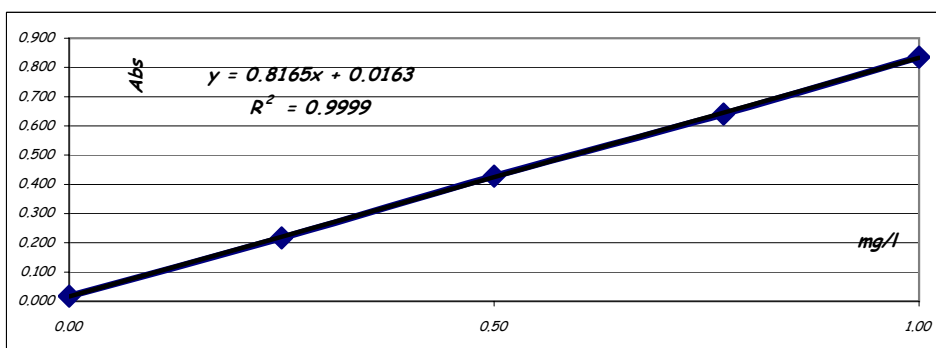

Test	Result	Specification	Pass / Fail
Intercept	0.0163	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8165	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes
 Store between 2 & 8 ° c
 *Stable on Board 5 days
 Barcode ID = 752
 *Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell