

Certificate of Performance

Sulphate Reagent



Product Code 984648  
984649  
Lot Number 8209

Date 20.10.2008


Expiry Date 14.10.2009

Reagent	Lot Number
Sulphate	8209
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.004
250	Sulp 4000 08 08	0.123
500	Sulp 4000 08 08	0.268
800	Sulp 4000 08 08	0.440
1000	Sulp 4000 08 08	0.540

\*serial Dilution

Calibration Curve

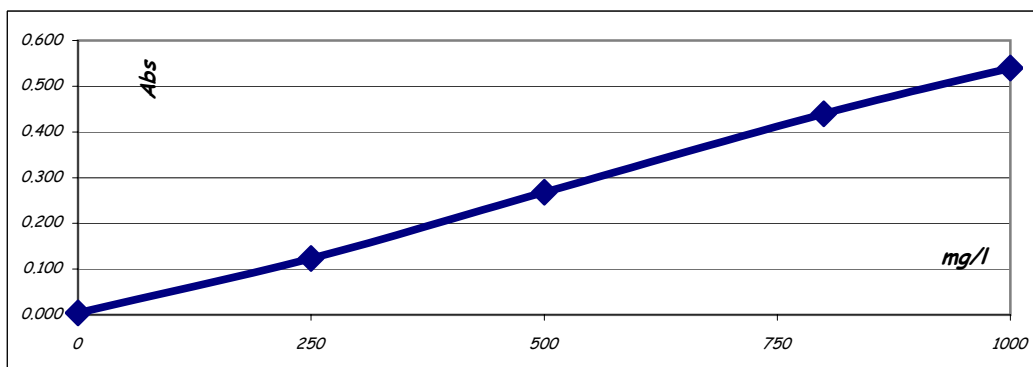

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm		
0 - 250 mg/l	0.0005	0.0003 to 0.0005	Pass
250 - 500 mg/l	0.0006	0.0003 to 0.0006	Pass
500 - 800 mg/l	0.0006	0.0004 to 0.0007	Pass
800 - 1000 mg/l	0.0005	0.0004 to 0.0008	Pass

Notes Store between 2 & 8 °c  
\*Stable on Board 5 days  
Barcode ID = 767  
\*Based on results obtained in our Research Facility

Dr. T. Russell