

Certificate of Performance

TON 3 Reagent



Product Code 984653  
984654  
Lot Number 8222

Date 03.12.2008


Expiry Date 10.11.2009

Reagent	Lot Number
TON 1	8182
TON 2	7245
TON 3	8222
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.003
2.50	TON 100 08 08	0.184
5.00	TON 100 08 08	0.362
7.69	TON 100 08 08	0.540
10.00	TON 100 08 08	0.677

\*serial dilution

Calibration Curve

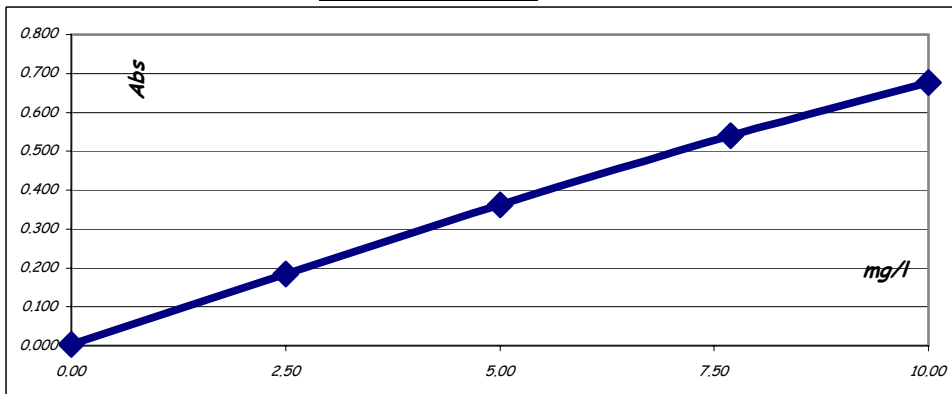

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
0 - 2.50 mg/l	0.0724	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0712	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0662	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0593	0.0500 to 0.0700	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board TON 1 - 1 day  
 \* TON 2 & TON 3 - 5 days  
 Keep Tightly Sealed when not in use.  
 Do not return unused portions to container  
 Barcode ID- TON 1 758; TON 2 759; TON 3 756  
 \* Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell