

Certificate of Performance

TON 3 Reagent



Product Code 984653
984654
Lot Number 8223

Date 03.12.2008


Expiry Date 10.11.2009

Reagent	Lot Number
TON 1	8133
TON 2	7245
TON 3	8223
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.001
2.50	TON 100 08 08	0.172
5.00	TON 100 08 08	0.348
7.69	TON 100 08 08	0.530
10.00	TON 100 08 08	0.655

*serial dilution

Calibration Curve

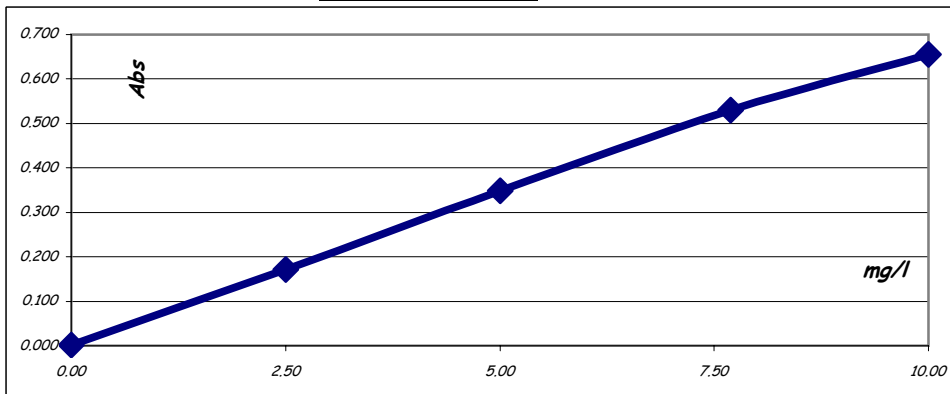

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
0 - 2.50 mg/l	0.0684	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0704	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0677	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0541	0.0500 to 0.0700	Pass

Notes Store between 2 & 8 °C
 *Stable on Board TON 1 - 1 day
 * TON 2 & TON 3 - 5 days
 Keep Tightly Sealed when not in use.
 Do not return unused portions to container
 Barcode ID- TON 1 758; TON 2 759; TON 3 756
 * Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell