

Certificate of Performance

**Amm 1 Reagent**



Product Code 984640

Lot Number 8238

Date 12.12.2008


Expiry Date 10.12.2009

Reagent	Lot Number
AMM 1	8238
Amm 2	8130
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.019
0.25	AMM 10 09 08	0.221
0.50	AMM 10 09 08	0.433
0.77	AMM 10 09 08	0.651
1.00	AMM 10 09 08	0.854

\*serial dilution

Calibration Curve

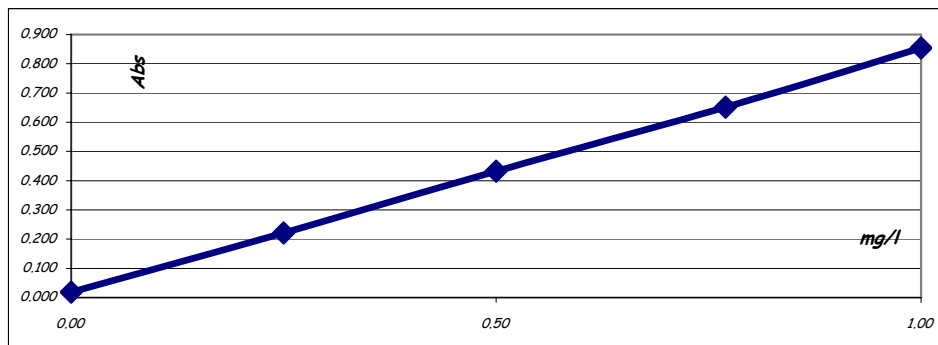

Test	Result	Specification	Pass / Fail
Intercept	0.0157	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8331	0.750 to 0.890	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes

Store between 2 & 8 ° c  
 \*Stable on Board 1 day  
 Barcode ID = 751  
 \*Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell