

Certificate of Performance

Phos 2 Reagent



Product Code 984645

984647

Lot Number 9001

Date 12.01.2009


Expiry Date 02.01.2010

Reagent	Lot Number
Phos 1	9005
Phos 2	9001
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 09 08	0.150
1	P20 09 08	0.294
1.5	P20 09 08	0.448
2	P20 09 08	0.579

*serial dilution

Calibration Curve

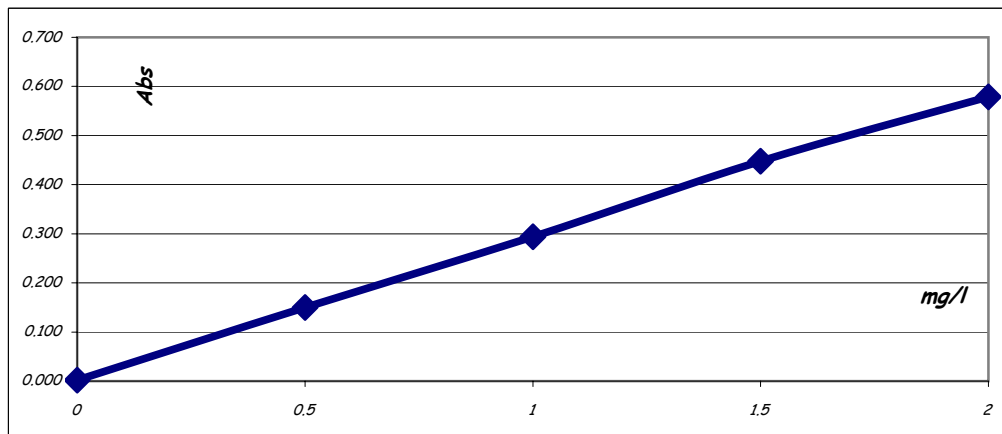

	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.290	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 765
* Based on results obtained in our Research Facility

Dr. T. Russell