

Certificate of Performance

Amm 2 Reagent



Product Code 984641

Lot Number 9002

Date 08.01.2009


Expiry Date 02.01.2010

Reagent	Lot Number
AMM 1	8205
Amm 2	9002
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	Amm 10 12 08	0.213
0.50	Amm 10 12 08	0.411
0.77	Amm 10 12 08	0.626
1.00	Amm 10 12 08	0.812

*serial dilution

Calibration Curve

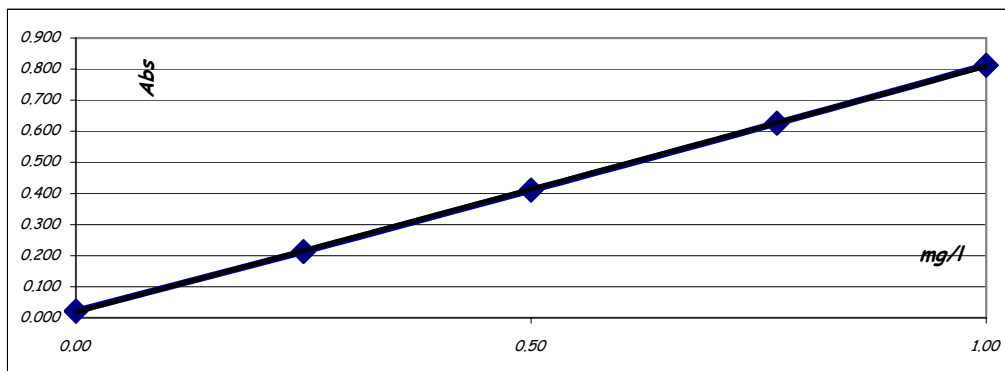

Test	Result	Specification	Pass / Fail
Intercept	0.0182	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7908	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °c
*Stable on Board 5 days
Barcode ID = 752
* Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell