

Certificate of Performance

TON 2 Reagent



Product Code 984651

984652

Lot Number 9015

Date 27.01.2009


Expiry Date 26.01.2010

| Reagent | Lot Number |
|-----------------|------------|
| TON 1 | 9014 |
| TON 2 | 9015 |
| TON 3 | 9016 |
| Test Method | LMTP03 |
| Test Instrument | Konelab 20 |
| Serial Number | P4919028 |

| Std. Value | Lot # | Abs. |
|------------|---------------|-------|
| 0.00 | | 0.003 |
| 2.50 | TON 100 12 08 | 0.186 |
| 5.00 | TON 100 12 08 | 0.356 |
| 7.69 | TON 100 12 08 | 0.520 |
| 10.00 | TON 100 12 08 | 0.648 |

*serial dilution

Calibration Curve

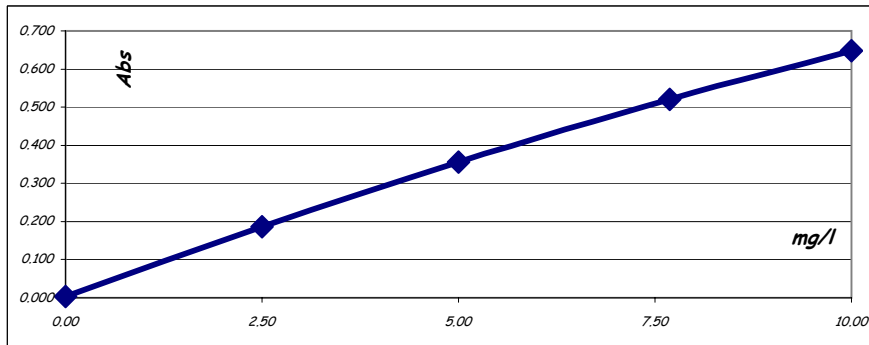

| Test | Result | Specification | Pass / Fail |
|------------------|---------|------------------|-------------|
| Intercept | 0.003 | -0.005 to 0.01 | Pass |
| Sensitivity | Abs/ppm | | |
| 0 - 2.50 mg/l | 0.0732 | 0.0550 to 0.0800 | Pass |
| 2.50 - 5.00 mg/l | 0.0680 | 0.0600 to 0.0800 | Pass |
| 5.00 - 7.69 mg/l | 0.0610 | 0.0550 to 0.0800 | Pass |
| 7.69 - 10.0 mg/l | 0.0554 | 0.0500 to 0.0700 | Pass |

Notes
Store between 2 & 8 °C
*Stable on Board TON 1 - 1 day
* TON 2 & TON 3 - 5 days
Keep Tightly Sealed when not in use.
Do not return unused portions to container
Barcode ID- TON 1 758; TON 2 759; TON 3 756
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell