

Certificate of Performance

**Amm 1 Reagent**



Product Code 984640  
Lot Number 9054

Date 20.03.2009


Expiry Date 18.03.2010

Reagent	Lot Number
AMM 1	9054
Amm 2	8130
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.024
0.25	AMM 10 12 08	0.209
0.50	AMM 10 12 08	0.407
0.77	AMM 10 12 08	0.616
1.00	AMM 10 12 08	0.805

\*serial dilution

Calibration Curve

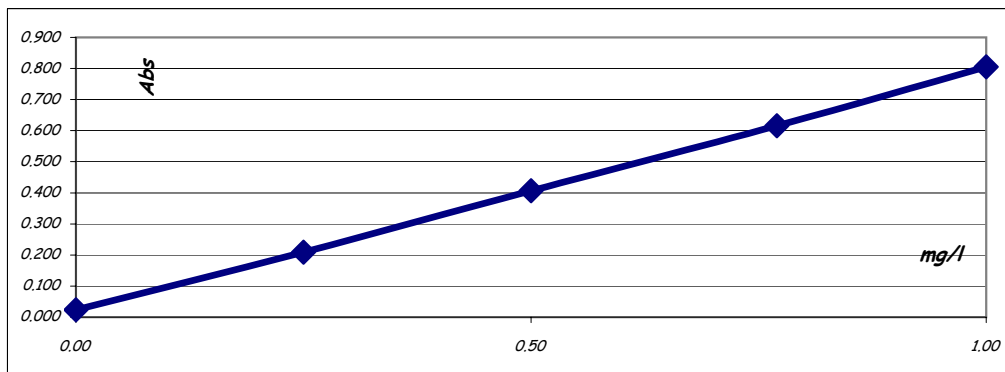

Test	Result	Specification	Pass / Fail
Intercept	0.0185	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7812	0.750 to 0.890	Pass
Regression	0.9997	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °c  
\*Stable on Board 1 day  
Barcode ID = 751  
\* Based on results obtained in our Research Facility

*Tom Russell.*  
Dr. T. Russell