

Certificate of Performance

TON 2 Reagent



Product Code 984651

984652

Lot Number 9076

Date 31.03.2009


Expiry Date 30.03.2010

Reagent	Lot Number
TON 1	8246
TON 2	9076
TON 3	8141
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.003
2.50	TON 100 12 08	0.181
5.00	TON 100 12 08	0.351
7.69	TON 100 12 08	0.515
10.00	TON 100 12 08	0.640

\*serial dilution

Calibration Curve

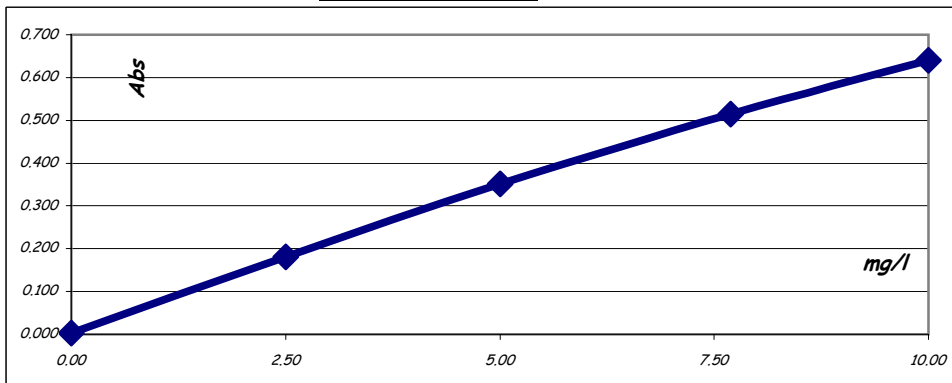

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity	Abs/ppm		
0 - 2.50 mg/l	0.0712	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0680	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0610	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0541	0.0500 to 0.0700	Pass

**Notes**  
Store between 2 & 8 °C  
\*Stable on Board TON 1 - 1 day  
\* TON 2 & TON 3 - 5 days  
Keep Tightly Sealed when not in use.  
Do not return unused portions to container  
Barcode ID- TON 1 758; TON 2 759; TON 3 756  
\* Based on results obtained in our Research Facility

Dr. T. Russell