

Certificate of Performance

Amm 2 Reagent



Product Code 984641

Lot Number 9097

Date 12.05.2009


Expiry Date 06.05.2010

Reagent	Lot Number
AMM 1	9096
Amm 2	9097
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.017
0.25	Amm 10 12 08	0.210
0.50	Amm 10 12 08	0.408
0.77	Amm 10 12 08	0.627
1.00	Amm 10 12 08	0.806

\*serial dilution

Calibration Curve

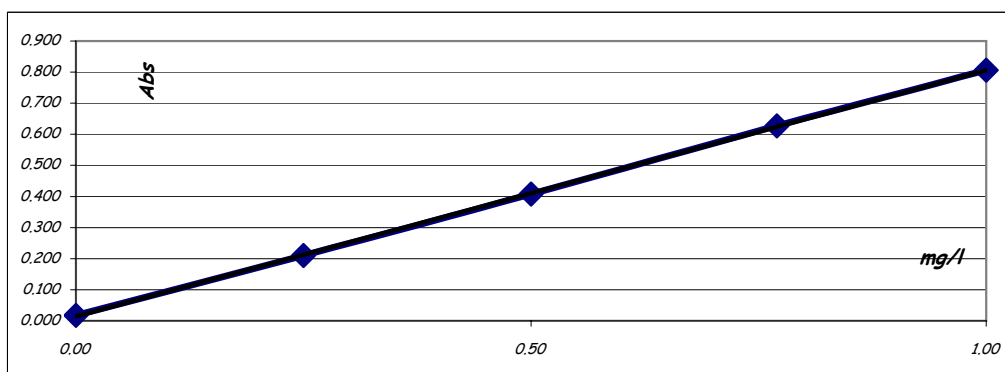

Test	Result	Specification	Pass / Fail
Intercept	0.0146	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7918	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes

Store between 2 & 8 °c

\*Stable on Board 5 days

Barcode ID = 752

\* Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell