

Certificate of Performance

Phos 2 Reagent



Product Code 984645

984647

Lot Number 9098

Date 13.05.2009


Expiry Date 06.05.2010

Reagent	Lot Number
Phos 1	9039
Phos 2	9098
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 01 09	0.146
1	P20 01 09	0.296
1.5	P20 01 09	0.455
2	P20 01 09	0.588

*serial dilution

Calibration Curve

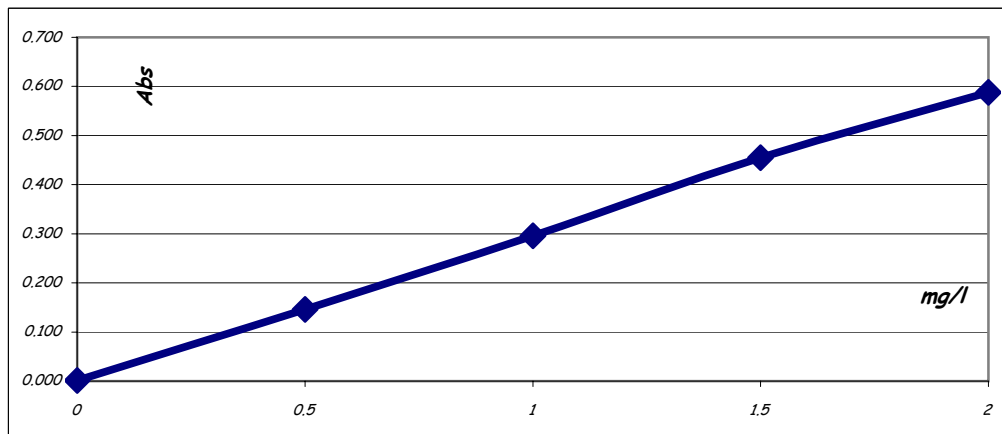

	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.297	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 765
* Based on results obtained in our Research Facility

Dr. T. Russell