

Certificate of Performance

Phos 1 Reagent



Product Code 984644

984646

Lot Number 9188

Date 12.10.2009


Expiry Date 08.10.2010

Reagent	Lot Number
Phos 1	9188
Phos 2	9035
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 08 09	0.142
1	P20 08 09	0.282
1.5	P20 08 09	0.441
2	P20 08 09	0.560

\*serial dilution

Calibration Curve

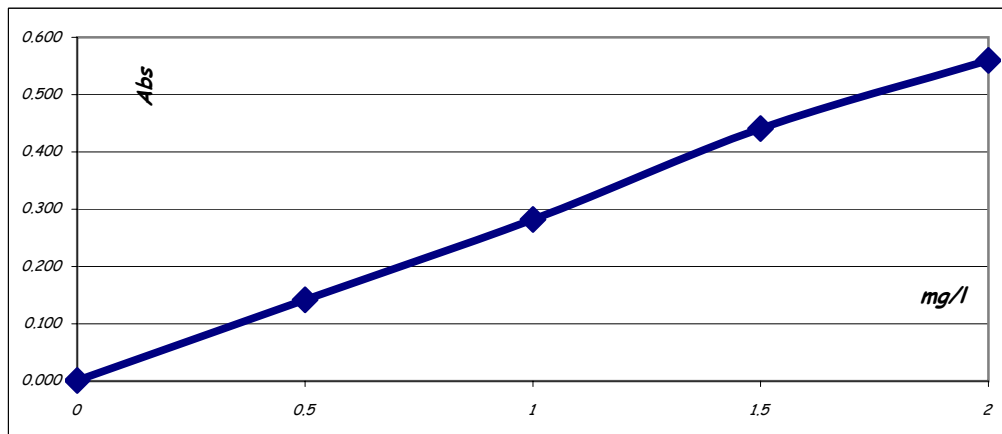

	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.283	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C  
\*Stable on Board 5 days  
Barcode ID = 763  
\* Based on results obtained in our Research Facility

Dr. T. Russell